

# **Precise Measurements of Small Linear and Angular Displacements with Capacitance Methods**

**Sergio Rescia**

- **Motivation: EDM G-2 Upgrade (by Gerald Bennet)**
- **Types of Displacement and Angle Sensors**
- **Advantages of Capacitive Displacement Sensors**
- **Readout Methods**
- **Limits to Sensitivity: Electrical and Mechanical Noise**
- **MEMS/Microelectronics Applications: Accelerometers**



**Acknowledgment:**

**The EDM Collaboration, especially G. Bennet, R. Burns, W. Morse, Y. Semertzidis, L. Snyderstrup**

**P. Rehak**

# Types of Displacement and Angle Sensors


## 1: Interferometric Sensor

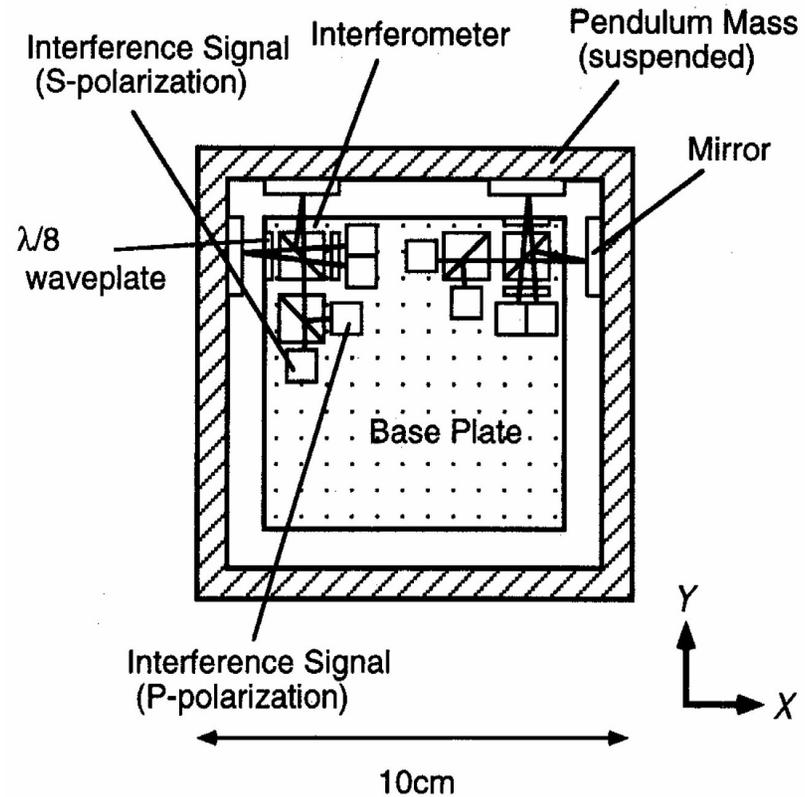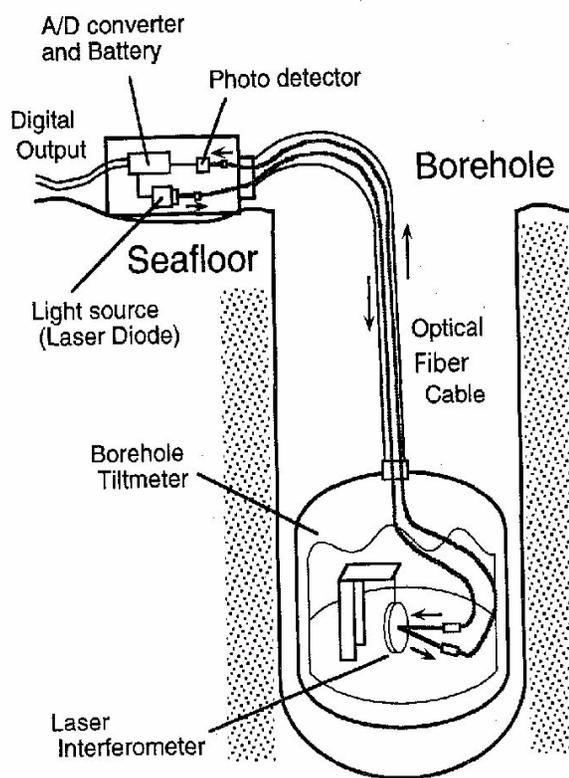

- **interferometric technique: optical wavelength-scale resolution**
- **Measures relative movements: laser light must be on all the time unless the reference point is lost**

# Types of Displacement and Angle Sensors

## 2: Interpolating Sensors (e.g SONY MAGNESCALE)


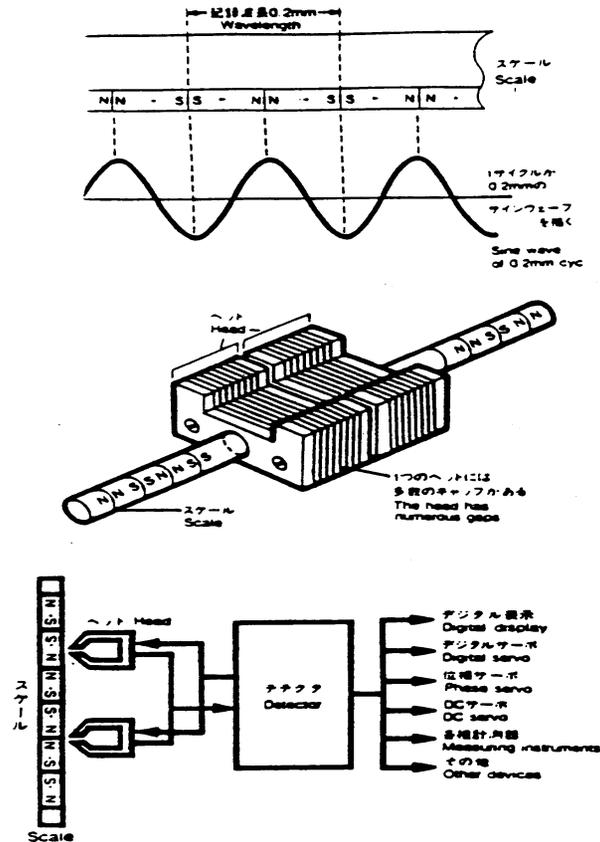


- Uses spatial averaging: reduced differential non-linearity
- Large Dynamic range
- Integral non-linearity depends on accumulated error in N-S magnetization locations

## Types of Displacement and Angle Sensors (cont)

### LVDT: Linear Variable Differential Transformer

A ferromagnetic core moves with respect to two opposite windings, changing the coupled flux.

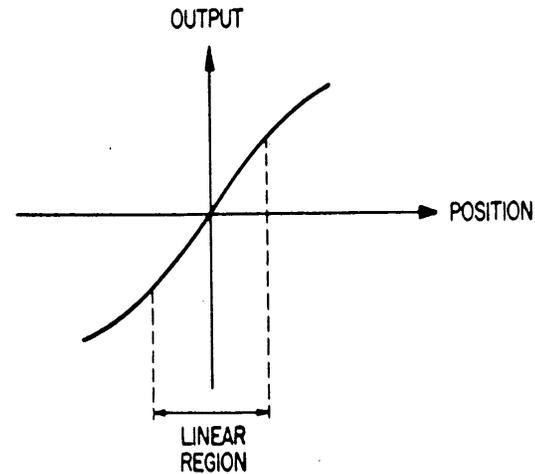
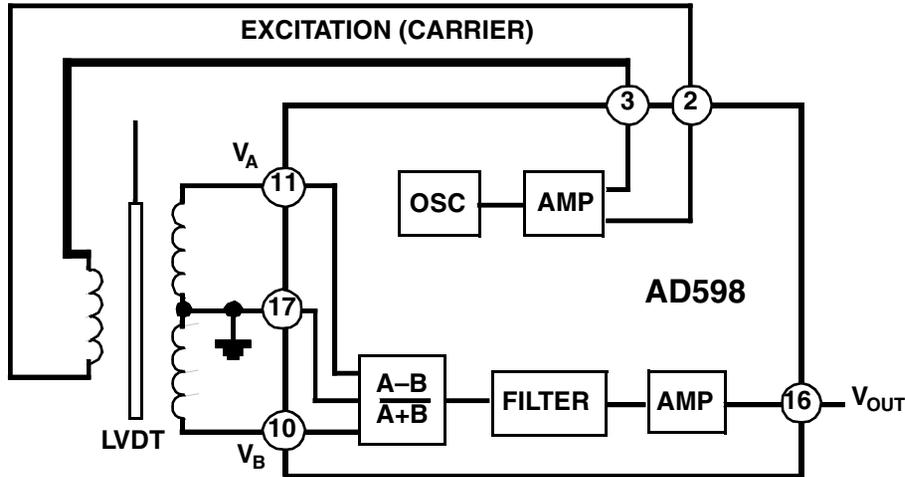


- S-shaped characteristics
- Bulky
- Slow response (uses low frequency)
- Sensitive to magnetic fields
- It is the most widely used displacement sensor



# Types of Displacement and Angle Sensors (cont)

## CAPACITIVE SENSORS

### Piston type variable Capacitor

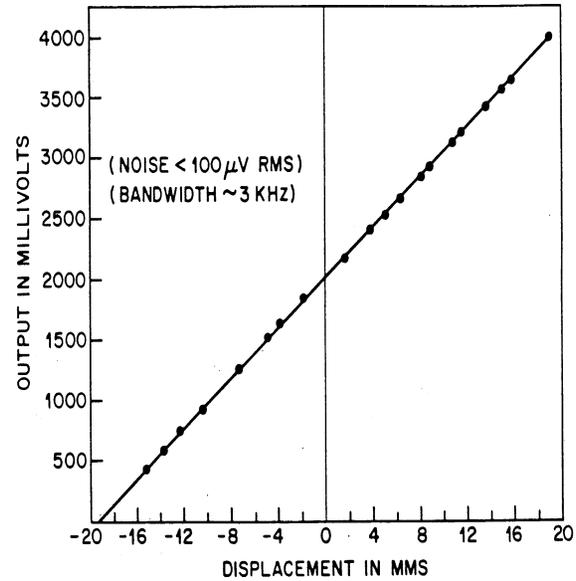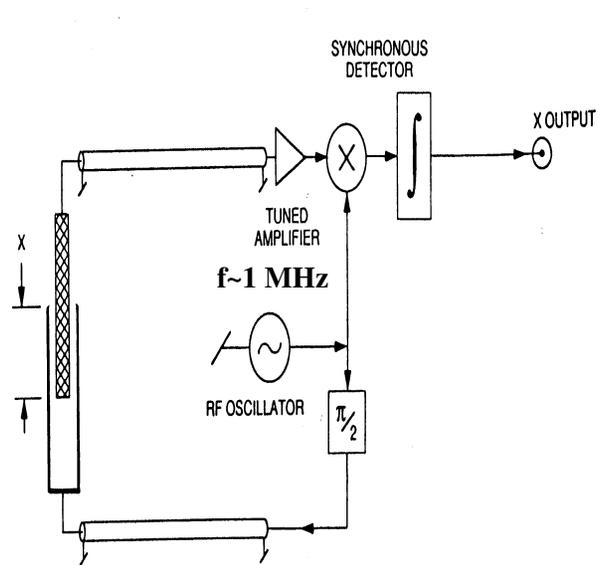

### Differential Capacitors

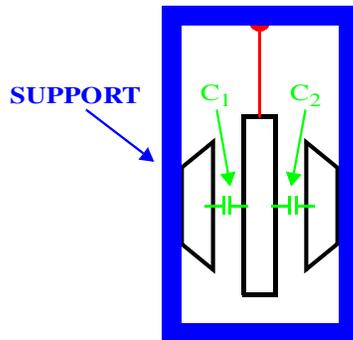

## Advantages of Capacitive Sensors

$$C = \epsilon \cdot \frac{A}{d}$$

Vary A => better linearity

Vary d => better sensitivity over small displacement



- **Excellent linearity over entire dynamic range when Area is changed (since stray electric fields are small)**
- **The system responds to average displacement of a large area of a moving electrode**
- **Freedom of electrode materials and geometry for demanding environments and applications**
- **Fractional change in capacitance can be made large**
- **Capacitive sensors can be made to respond to displacements in one direction only**
- **The forces exerted by the measuring apparatus are electrostatic, and usually small enough so that they can be disregarded**
- **Capacitors are noiseless: excellent S/N ratio can be obtained (or their dissipation factor D is large enough that the dominant noise sources are elsewhere)**

# Types of Readout

## Two major categories:

1. Readout based on Resonance
2. Readout based on Bridge method

## Readout based on Resonance

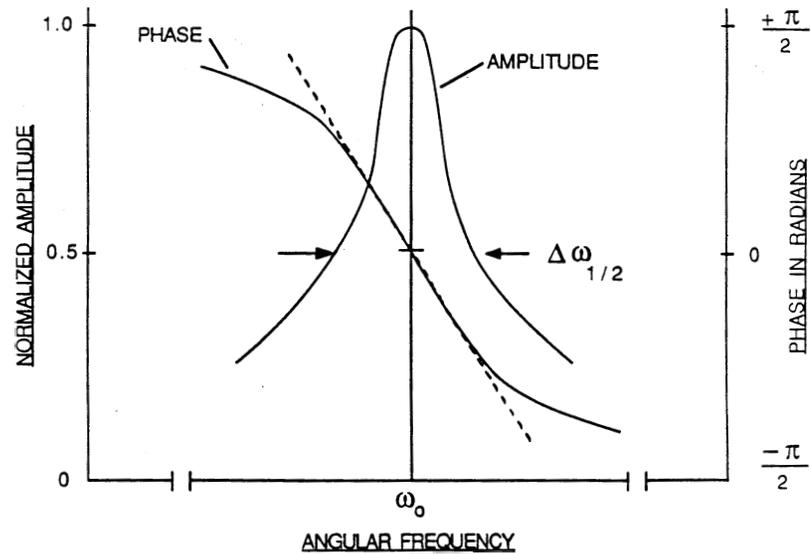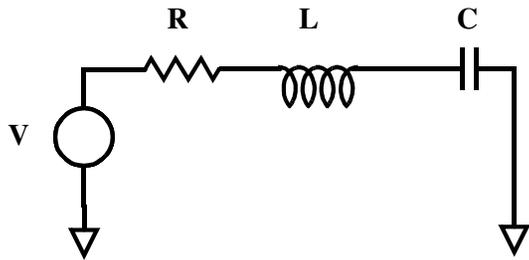

1. Measure frequency change of an oscillator built around the variable capacitor
1. Excite at resonance, measure amplitude change
2. Excite at resonance, measure phase change
3. Use feedback loop and VCO oscillator to track resonance change

## **Readout based on Resonance (cont)**

### **Advantages**



- **Makes use of the high Q of a resonant circuit: does not require a low noise preamplifier**
- **Sensitive**
- **Simple and straightforward**

### **Disadvantages**


- **All resonating elements are created equal: it cannot distinguish a change in L from a change in C.  
The overall stability depends on the stability of BOTH L and C, with different temperature coefficients and stray effects.**
- **Cannot take advantage of differential capacitance change**

# Readout Based on Resonance: Example

## Rocking Beam Balancing in Atomic Force Microscope (G. L. Miller)

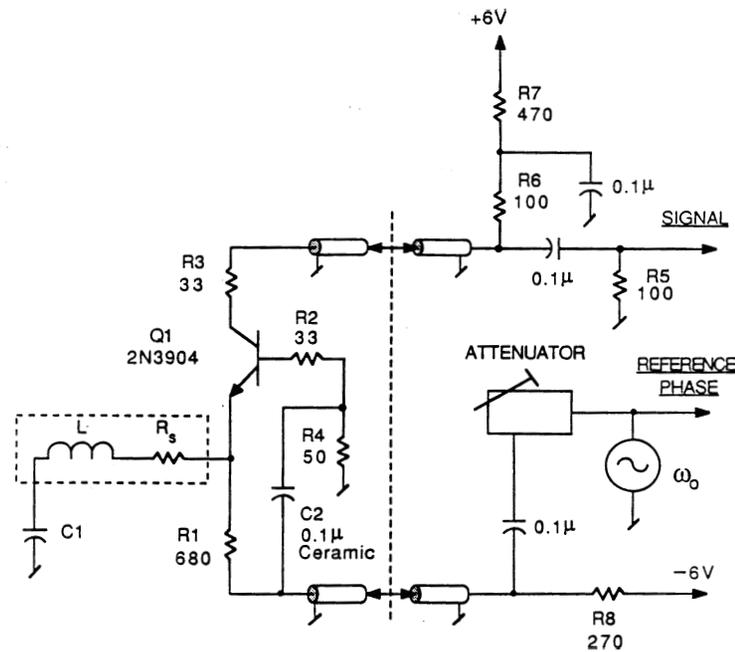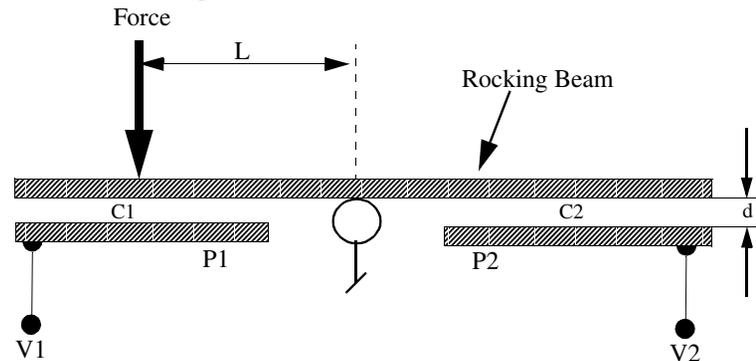

## Types of Readout: AC Bridge

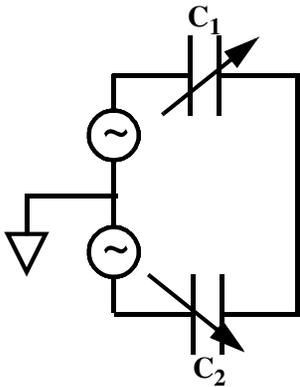

$$C_1 - C_2 = \epsilon A / (\delta x - x_0) - \epsilon A / (\delta x + x_0) = 2 C_0 \delta x / x_0$$


$$A = 400 \text{ mm}^2 \quad x_0 = 75 \text{ } \mu\text{m} \quad C_1 = C_2 = 50 \text{ pF}$$

$$l = 30 \text{ mm} \quad \delta\theta = 1 \text{ nrad} \quad \delta x = \delta\theta l = 30 \cdot 10^{-12} \text{ m}$$

$$\delta C = C_1 - C_2 = 40 \text{ aF}$$


$$\text{Force} = \frac{1}{2} \cdot \frac{C_1}{x_0} \cdot V_1^2$$

**F = 0 for a symmetric system**

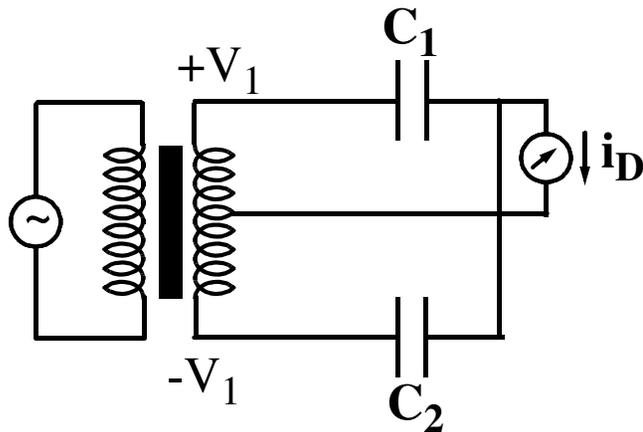

$$i_D = V_1 \omega (C_1 - C_2)$$

## Types of Readout: AC Bridge Readout Equivalent Circuit

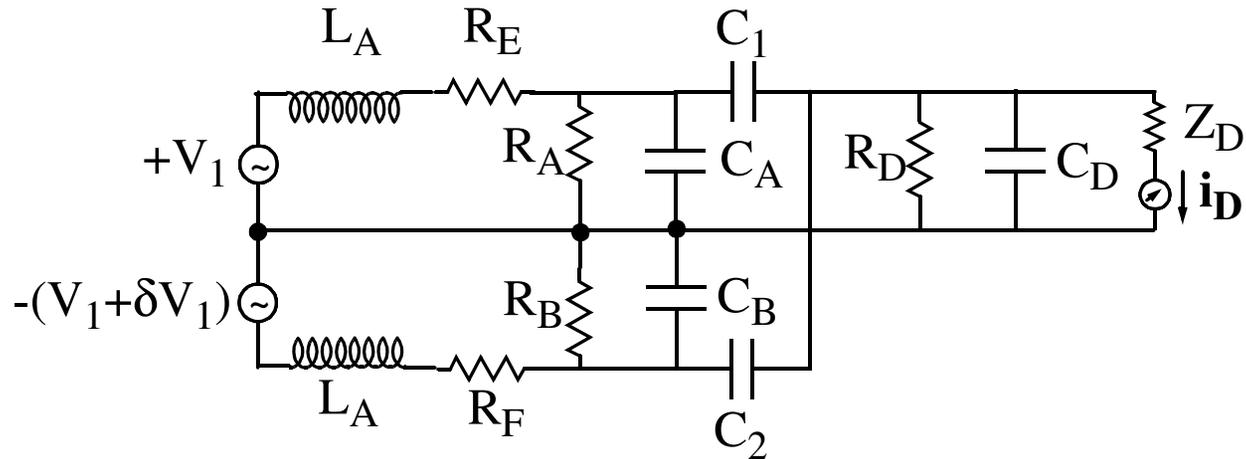


**For zero output from the capacitance balance detector must be:**

$$\frac{C_1}{C_2} = 1 + L_B(C_2 + C_B)\omega^2 - L_A(C_1 + C_A)\omega^2 + \frac{R_E}{R_A} - \frac{R_F}{R_B} + \frac{\delta V_1}{V_1}$$


$L_A, L_B$	0.4 mH	ratio transformer Leakage inductance
$R_E, R_F$	<1 $\Omega$	transformer secondary DC resistance
$R_A, R_B$	>10 M $\Omega$	Dielectric losses
$C_A, C_B$	~ 1000 pF	Stray capacitance to "ground" (cables, interwinding C)
$R_D, C_D$		Impedance shunting the preamplifier. Does not affect balance
$Z_D$	low	Current preamplifier input impedance

# Readout Circuit

## EXCITATION

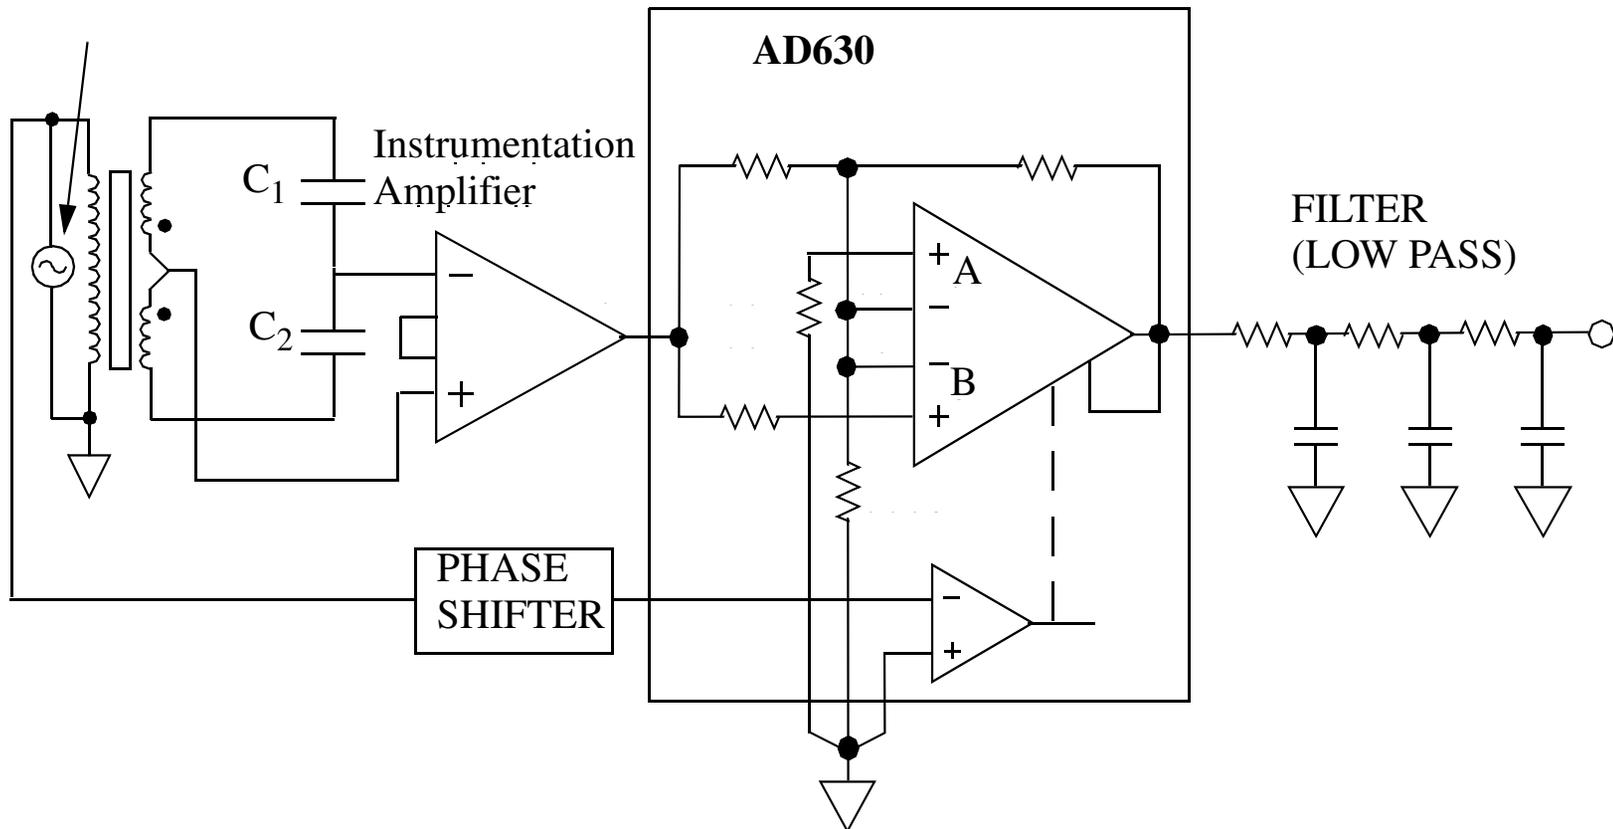

## AC Bridge: Noise

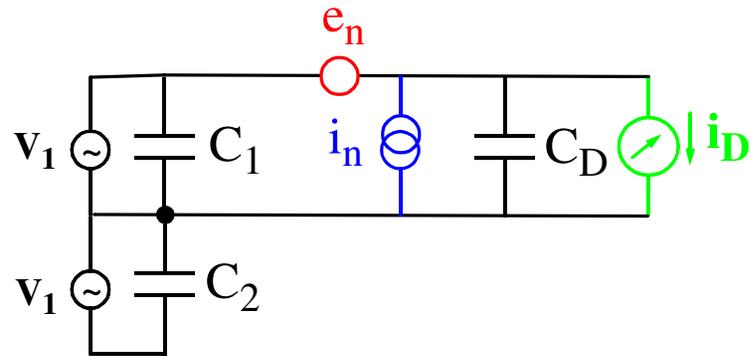

$$\overline{i_{D,n}^2} = \left( \overline{i_n^2} + \frac{\overline{e_n^2}}{1/\omega_0^2 C_T^2} \right) BW$$

$$C_T = C_1 + C_2 + C_D$$

The “equivalent noise capacitance” can be calculated as:

$$\left( \overline{i_n^2} + \frac{\overline{e_n^2}}{1/\omega_0^2 C_T^2} \right) BW = \frac{V_1^2}{1/(\omega_0^2 C_n^2)}$$

so that we have:

$$\overline{C_n^2} = \frac{1}{V_1^2} \left( \overline{e_n^2} C_T^2 + \frac{\overline{i_n^2}}{\omega_0^2} \right) BW$$

## AC Bridge: Noise (cont)

To reduce noise:

- Increase  $V_1$
- Decrease Bandwidth (i.e. increase averaging time)
- Decrease  $C_T$  (depends mostly on connection length, strays etc.)

Example: Tiltmeter

$$\left. \begin{array}{l} C_T = 1 \text{ nF} \\ e_n = 1 \text{ nV/Hz}^{1/2} \\ V_1 = 3 \text{ V} \end{array} \right\} C_n = 4 \cdot 10^{-19} \text{ F} = 400 \text{ zF}$$

Minimum Signal (for 1 nrad angular displacement) = 40 aF =  $20 \cdot 10^{-18} \text{ F}$   $\Rightarrow$  S/N=100

Example: Monolithic MEMS circuit

$$\left. \begin{array}{l} C_T = 1 \text{ pF} \\ e_n = 10 \text{ nV/Hz}^{1/2} \\ V_1 = 5 \text{ V} \end{array} \right\} C_n = 2 \cdot 10^{-21} \text{ F} = 2 \text{ zF}$$

# Mechanical Noise

The mechanical rms fluctuation can be computed by means of the fluctuation dissipation theorem.  
The rms fluctuation of the displacement of a suspended mass  $m$  is:

$$\overline{\delta x^2} \equiv \frac{k_B T}{m \omega_0^2 \tau S}$$

Where:

$$k_B = 1.38 \cdot 10^{-23} \text{ J/K}$$

$$m \sim 20 \text{ g}$$

$$\omega_0 = \text{mechanical resonant frequency} \sim 10^5 \text{ rad/sec}$$

$$\tau = \text{damping time constant} \sim 5\text{-}10 \text{ sec}$$

$$S = \text{Averaging period} \sim 1 \text{ sec to minutes}$$

So that  $(\delta x^2)^{(1/2)} \sim 10^{-17} \text{ m}$  giving a “noise” too small to be detected.

**Absolute Limits:**

Since the averaging  $S$  and damping time constant  $\tau$  could be increased (e.g. mounting the tiltmeter in vacuum to reduce friction and reducing the mechanical losses of the hinge) there is no fundamental limit to the mechanically generated noise.

## Other Sources of Errors

- **Temperature variations**

**Thermal expansion => cancelled in a symmetrical design**

**Effects on the readout electronics: Gain Variation**

**temperature dependence of dielectric constant ( $2 \cdot 10^{-6}/^{\circ}\text{C}$  for dry air at STP;**

**$700 \cdot 10^{-6}$  for moist air**

- **Humidity variations**

**at  $20^{\circ}\text{C}$  a change in humidity from 40 to 90% changes the dielectric constant by 200 ppm**

- **Pressure changes**

**a pressure change of 1 atm at  $20^{\circ}\text{C}$  changes the dielectric constant by 200 ppm**

**causes dimensional changes (a brass cube of 1 cm contracts by  $3 \mu\text{m}$  for a 1 atm change)**

- **Oxidation of surfaces (rodium plating recommended)**



- **Stability of materials (70-30 brass gives good results)**

- **Creep of materials**

- **Relaxation of screw tension**

- **Microseismicity (about  $2 \mu\text{m}$  peak to peak displacement, period 3-8 s)**

# MEMS Accelerometers

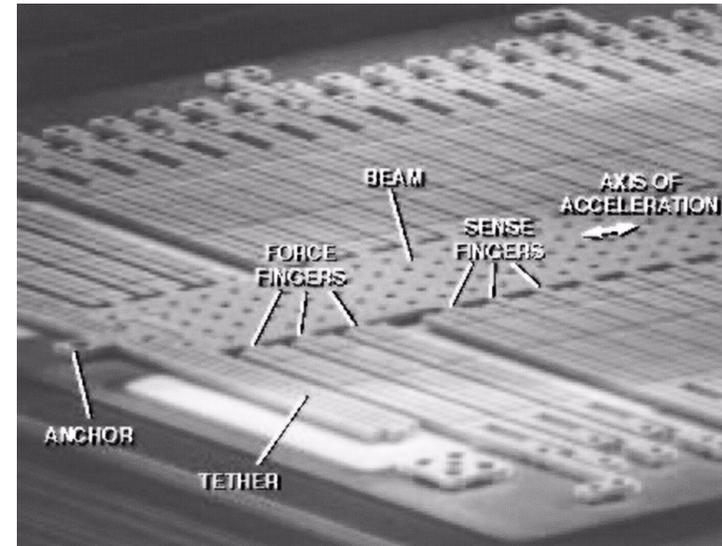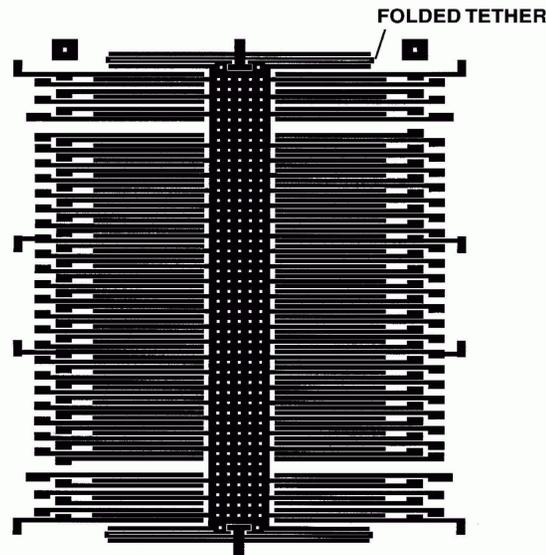

It consist of multiple fingers on each side of a movable center member.

They constitute the center plates of a paralleled set of differential capacitors. Pairs of fixed fingers attached to the substrate interleave with the beam fingers to form the outer capacitor plates. The beam is supported by tethers which serve as mechanical spring.

“Force” fingers are used for calibration


mass =  $0.5 \mu\text{g}$

SIZE:  $0.5 \text{ mm} \times 0.4 \text{ mm}$ ,  $2 \mu\text{m}$  thick,

- Requirement: Avoid “stiction” => rigid cantilevered beam


# Sensor operation; ADI's implementation

- **Folded tethers have more consistent spring constants, leading to better part to part consistency**

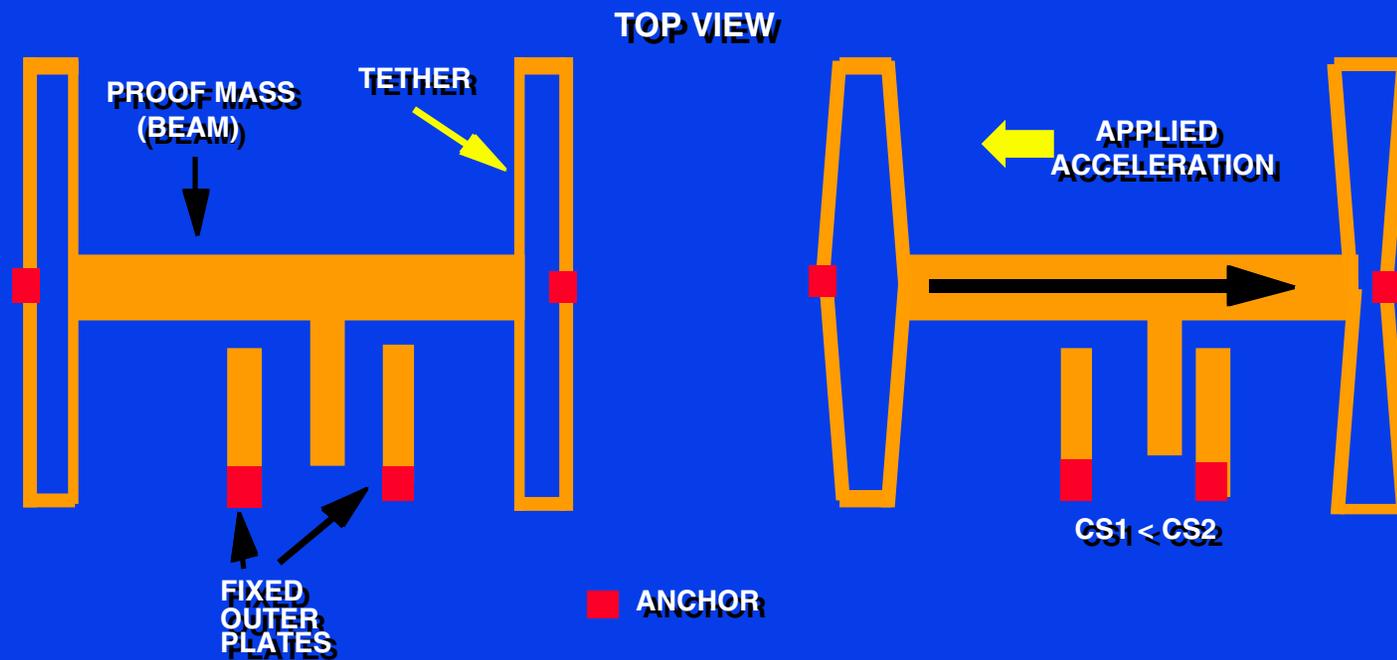

# Self test operation

- Extra fixed outer plates may be added which when excited, force the proof mass to move. So you can electronically test the accelerometer

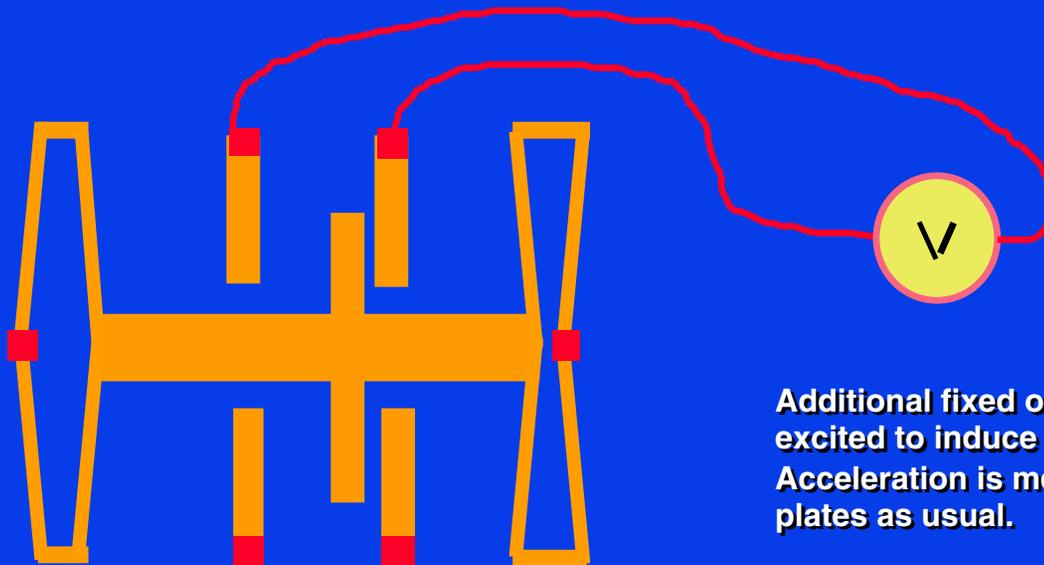

Additional fixed outer plates are electrically excited to induce movement of the proof mass. Acceleration is measured by the standard fixed plates as usual.



# Interesting facts



- **0.1 $\mu$ grams Proof Mass**
- **0.1pF per Side for the Differential Capacitor**
- **20aF ( $10^{-18}$ f) Smallest Detectable Capacitance Change**
- **Total Capacitance Change for Full-scale is 10fF**
- **1.3 $\mu$ m Gaps Between Capacitor Plates**
- **0.2 $\text{\AA}$  Minimum Detectable Beam Deflection (one tenth of an Atomic diameter)**
- **1.6  $\mu$ m Between the Suspended Beam and Substrate**
- **10 to 22kHz Resonant Frequency of Beam**

# MEMS Accelerometers:

## Readout

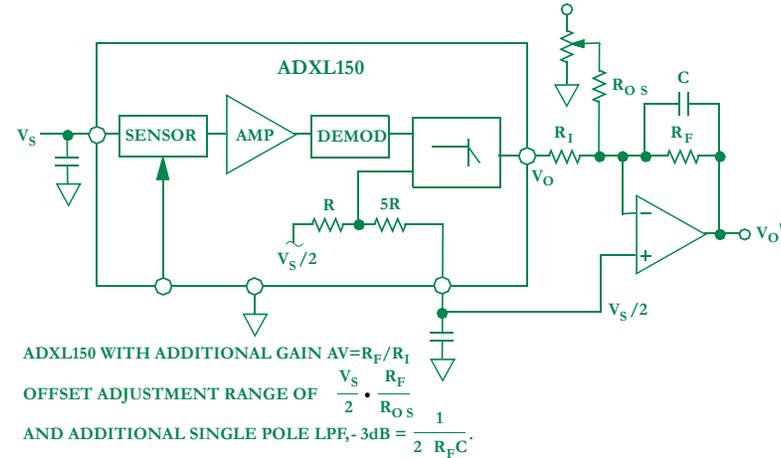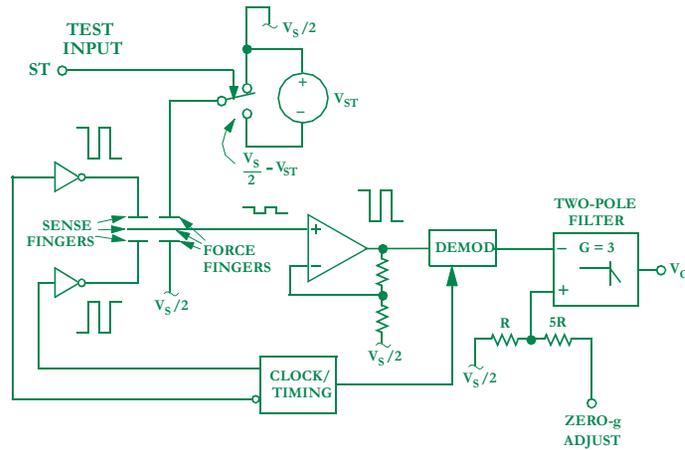

## Noise

Specifications	ADXL105	ADXL202	ADXL05	ADXL50
Range	$\pm 5 g$	$\pm 2 g$	$\pm 5 g$	$\pm 50 g$
Noise ( $\mu g / \sqrt{Hz}$ )	225	500	500	6500
Bandwidth (kHz)	10	5	5	6
Supply Current (mA)	2	0.6	10	10
Number of Axes	1	2	1	1
Output Type	Analog	Analog/ Digital	Analog	Analog

### ADXL105:

$C = 150 \text{ fF}$

Sensitivity = 100 aF for 1g acceleration

noise = 225 g/Hz<sup>1/2</sup>

“capacitance” noise =  $22.5 \cdot 10^{-21} \text{ F/Hz}^{1/2} = 22.5 \text{ zF/Hz}^{1/2}$

## Bibliography

1. G.L. Miller “Sensor and actuators for small motions”, unpublished report available from S. Rescia
2. R.V. Jones and C. S. Richards, “The design and some application of sensitive capacitance micrometers”, J. Phys. E 6, 589 (1973)
3. A. M. Thomson, “The precise measurements of small capacitances”, IRE Trans. Instrum, I-7, 245 (1958)
4. G. L. Miller, E. R. Wagner and T. Sleator, “Resonant phase technique for the measurement of small changes in grounded capacitors”, Rev. Sci. Instrum., 61 (4), 1287 (1990)
5. H. W. Callen and R. F. Greene, “On a theorem of irreversible thermodynamics”, Phys. Rev., 86 (5), 702 (1952)
6. P. S. Saulson, “Thermal noise in mechanical experiments”, Phys. Rev. D 42, 2437 (1990)
7. A good tutorial on random noise in mechanical system as applied to gravitational wave antennas is in P. S. Saulson “Physics of gravitational wave detection: resonant and interferometric detectors” available at “<http://www.astro.psu.edu/users/steinn/Astro597/saulson.pdf>”
8. A good reference book on the art of winding of ratio transformers and high precision AC bridge techniques is the book “Coaxial AC Bridges” by Brian Kibble and G. Rayner, published by Bristol A. Hilger, 1984. It is out of print, but a photocopy can be ordered through the UK National Physical Laboratory at the URL: <http://www.npl.co.uk/electromagnetic/cem-publications/goodpractice.html>